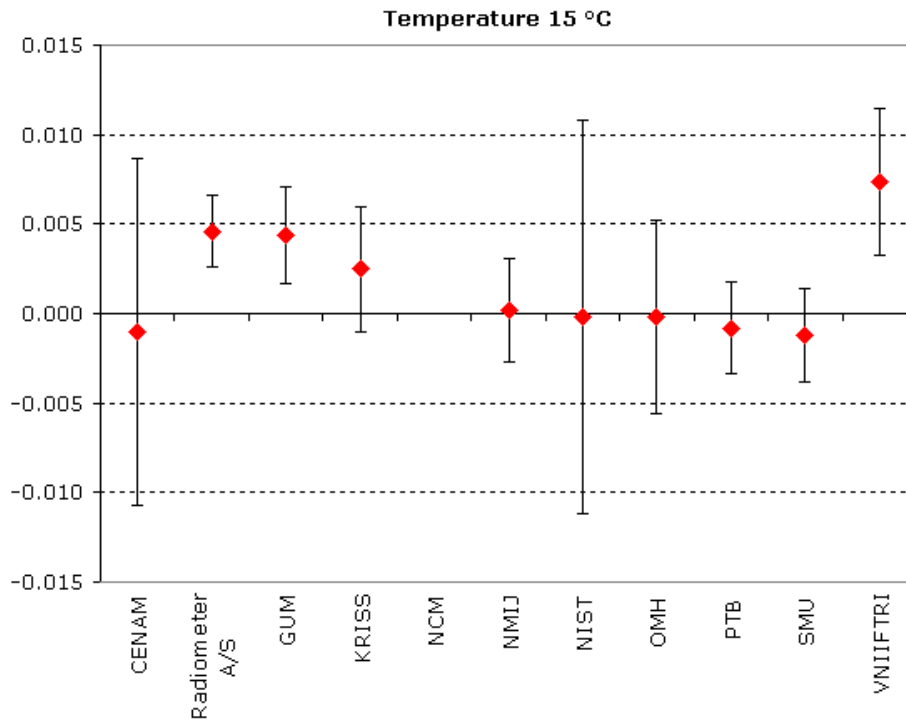



MEASURAND : Acidity function at zero chloride molality of an unknown borate buffer, pH ~ 9.17

TEMPERATURE : 15 °C

Degrees of equivalence D_i and expanded uncertainty U_i ($k = 2$)

MEASURAND : Acidity function at zero chloride molality of an unknown borate buffer, pH ~ 9.17

TEMPERATURE : 25 °C

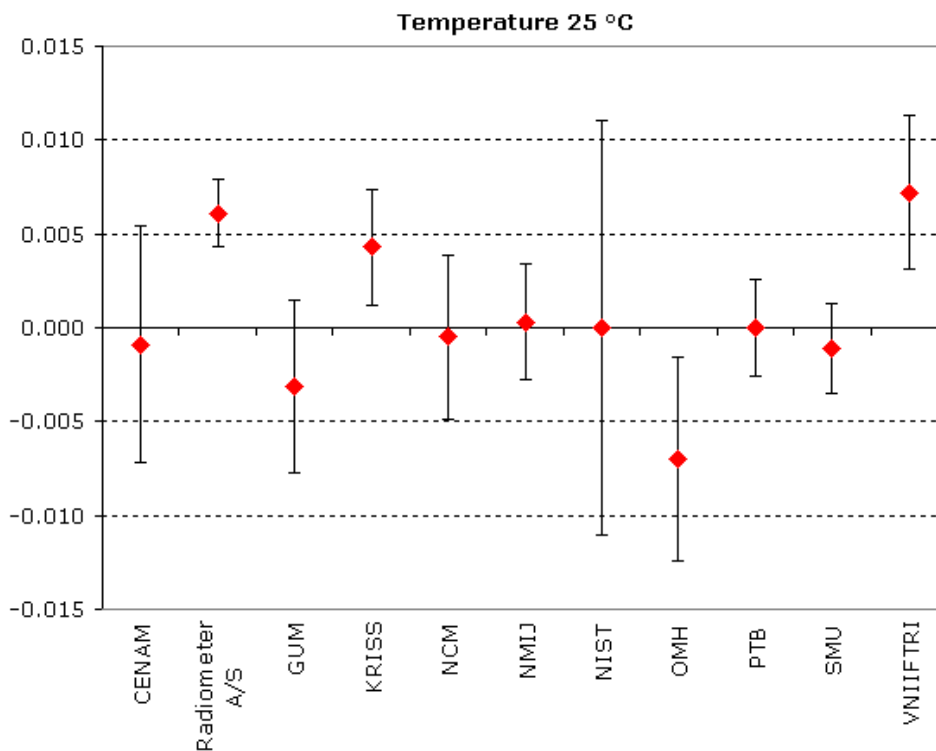Degrees of equivalence D_i and expanded uncertainty U_i ($k = 2$)

MEASURAND : Acidity function at zero chloride molality of an unknown borate buffer, pH ~ 9.17

TEMPERATURE : 37 °C

Degrees of equivalence D_i and expanded uncertainty U_i ($k = 2$)

