


MEASURAND : Mass fraction of Phenanthrene in solution  
NOMINAL VALUE : 5473 ng/g

Offset  $D_i = (x_i - x_R)$  and expanded uncertainty  $U_{\text{Lab } i}$  (95% level of confidence)  
of each laboratory  $i$  both expressed in (ng/g)


$x_R = 5473 \text{ ng/g}$  and  $U_R = 141 \text{ ng/g}$

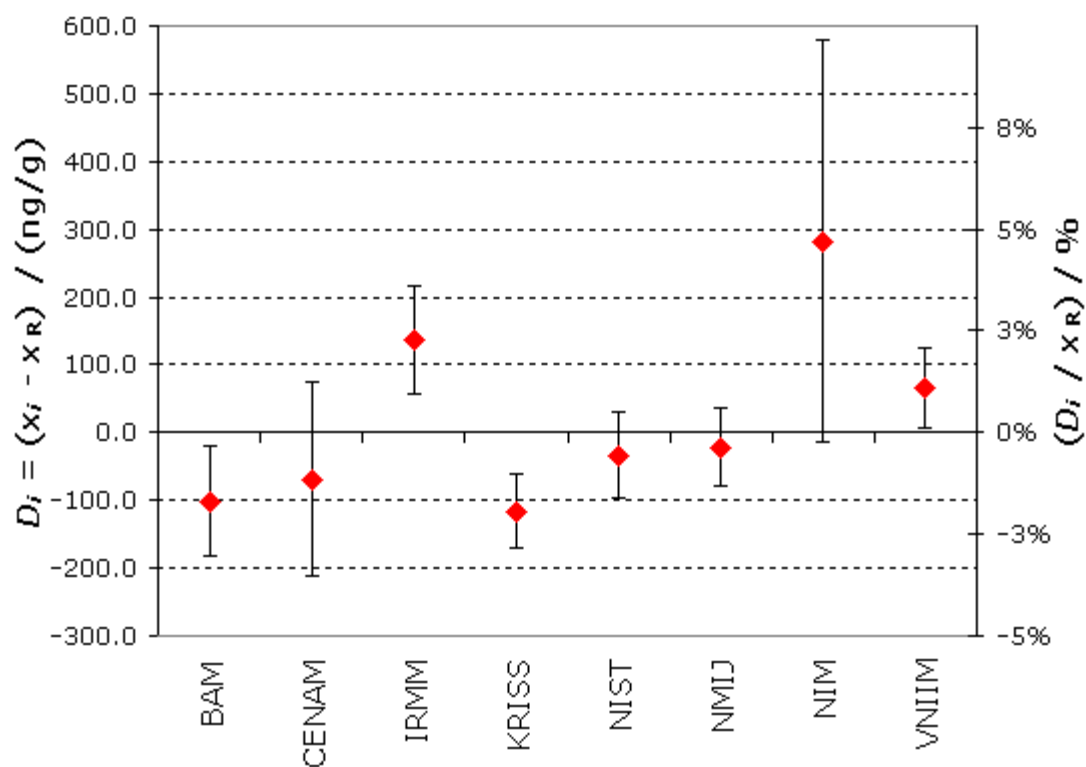

MEASURAND : Mass fraction of Fluoranthene in solution  
NOMINAL VALUE : 8906 ng/g

Offset  $D_i = (x_i - x_R)$  and expanded uncertainty  $U_{Lab\ i}$  (95% level of confidence) of each laboratory  $i$  both expressed in (ng/g)


$x_R = 8906$  ng/g and  $U_R = 196$  ng/g

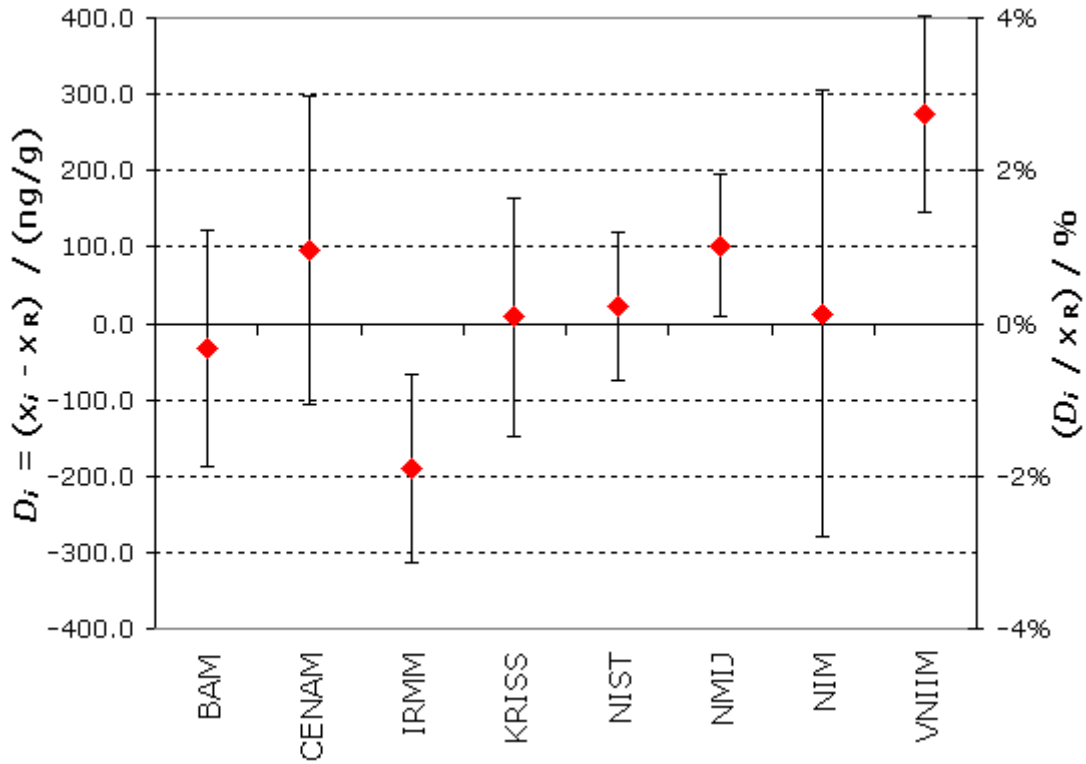

MEASURAND : Mass fraction of Benz[a]anthracene in solution  
NOMINAL VALUE : 3952 ng/g

Offset  $D_i = (x_i - x_R)$  and expanded uncertainty  $U_{Lab, i}$  (95% level of confidence) of each laboratory  $i$  both expressed in (ng/g)


$x_R = 3952$  ng/g and  $U_R = 95$  ng/g

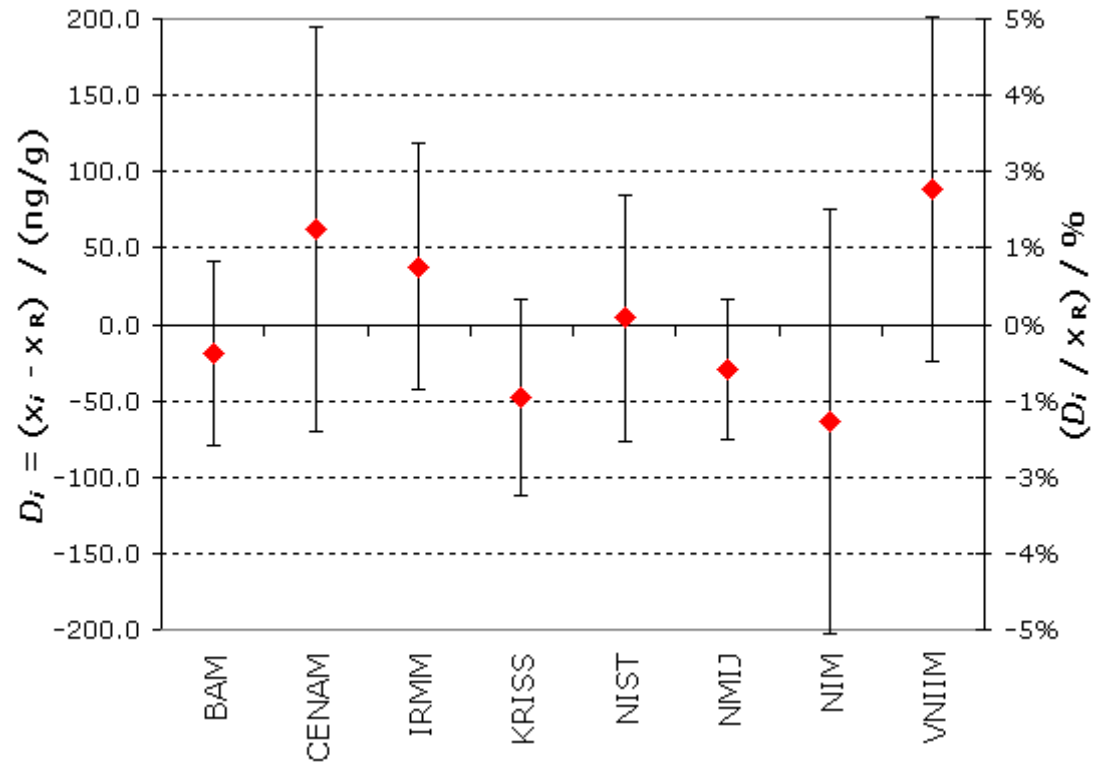

MEASURAND : Mass fraction of Benzo[a]pyrene in solution  
NOMINAL VALUE : 4956 ng/g

Offset  $D_i = (x_i - x_R)$  and expanded uncertainty  $U_{Lab\ i}$  (95% level of confidence) of each laboratory  $i$  both expressed in (ng/g)

$x_R = 4956$  ng/g and  $U_R = 153$  ng/g

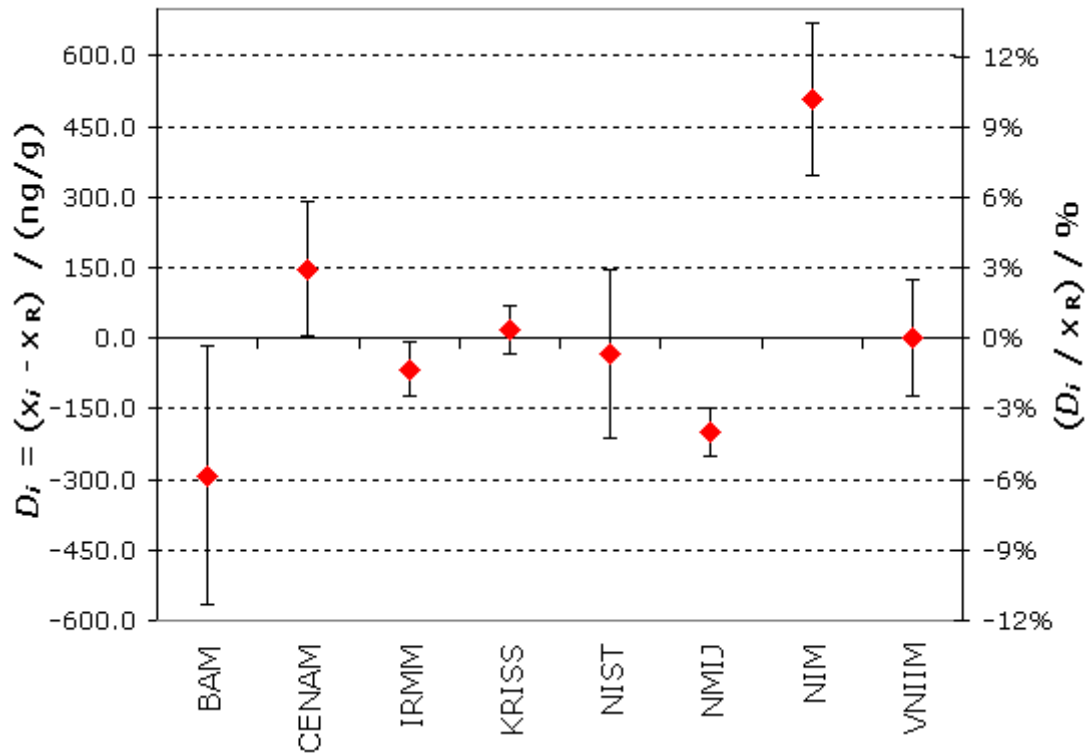

MEASURAND : Mass fraction of Benzo[ghi]perylene in solution  
NOMINAL VALUE : 6872 ng/g

Offset  $D_i = (x_i - x_R)$  and expanded uncertainty  $U_{Lab, i}$  (95% level of confidence) of each laboratory  $i$  both expressed in (ng/g)

$x_R = 6872$  ng/g and  $U_R = 146$  ng/g

